


ARKival Technology REV 2013031401-VSM-ONE  
Filename: exp\_19\_p Sample ID:Exponent 810-03919/p  
Vibrating Sample Magnetometer - Hysteresis loop data array  
Date Run: 29 Jan 2017 Time Run: 12:49:49

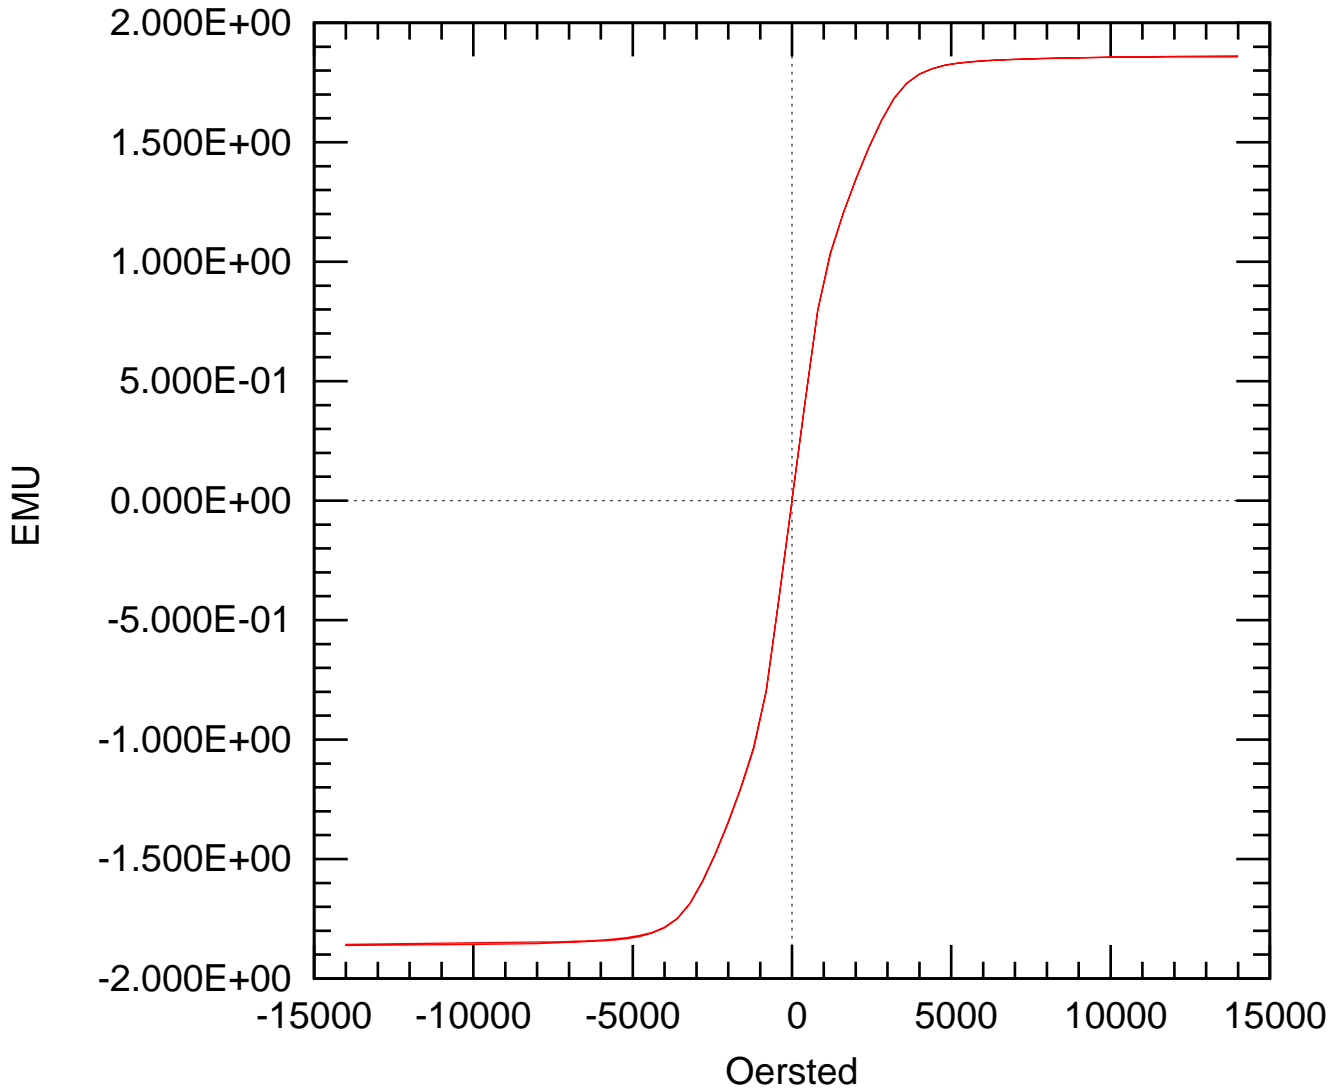

Hmax = 1.400E+04  
Is = 1.857E+00  
Ir = 3.202E-03  
SQ = 1.724E-03

Mass = 2.030E-02  
Hc = 3.502E+00  
dH = 3.092E+00  
SFD = 8.831E-01